



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

1 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
Permanent Facility				
1	CLINICAL BIOCHEMISTRY	EDTA Plasma	Interleukin-6	CLIA
2	CLINICAL BIOCHEMISTRY	EDTA Whole Blood	Glycosylated Haemoglobin	Immunoturbidimetry
3	CLINICAL BIOCHEMISTRY	EDTA Whole Blood	Troponin - T	Immunochemistry
4	CLINICAL BIOCHEMISTRY	EDTA Whole Blood/Serum/EDTA Plasma	Troponin - I	Membrane based immunoassay
5	CLINICAL BIOCHEMISTRY	Plasma/CSF/Ascitic Fluid/Pleural Fluid/Synovial Fluid/Pericardial Fluid/	Glucose	Hexokinase
6	CLINICAL BIOCHEMISTRY	Serum	17 Alpha Hydroxy Progesterone	ELISA
7	CLINICAL BIOCHEMISTRY	Serum	ADA	Kinetic colorimetry
8	CLINICAL BIOCHEMISTRY	Serum	Alanine aminotransferase	UV Without P5P
9	CLINICAL BIOCHEMISTRY	Serum	Albumin	Bromo cresol green
10	CLINICAL BIOCHEMISTRY	Serum	Albumin	Gel Electrophoresis
11	CLINICAL BIOCHEMISTRY	Serum	Albumin / Globulin Ratio	Calculated
12	CLINICAL BIOCHEMISTRY	Serum	Alfa Feto Protein	Electro Chemiluminescence
13	CLINICAL BIOCHEMISTRY	Serum	Alkaline phosphatase	IFCC
14	CLINICAL BIOCHEMISTRY	Serum	Alpha-1	Gel Electrophoresis
15	CLINICAL BIOCHEMISTRY	Serum	Alpha-2	Gel Electrophoresis
16	CLINICAL BIOCHEMISTRY	Serum	Anti CCP	CLIA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

2 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
17	CLINICAL BIOCHEMISTRY	Serum	Anti Mullerian Hormone	Chemiluminescence
18	CLINICAL BIOCHEMISTRY	Serum	Anti Thyroglobulin Antibody	Chemiluminescence
19	CLINICAL BIOCHEMISTRY	Serum	Anti TPO	Chemiluminescence
20	CLINICAL BIOCHEMISTRY	Serum	Aspartate aminotransferase	IFCC Without P5P
21	CLINICAL BIOCHEMISTRY	Serum	Beta	Gel Electrophoresis
22	CLINICAL BIOCHEMISTRY	Serum	Bilirubin direct	Diazo
23	CLINICAL BIOCHEMISTRY	Serum	Bilirubin indirect	Calculated
24	CLINICAL BIOCHEMISTRY	Serum	Bilirubin total	Diazo
25	CLINICAL BIOCHEMISTRY	Serum	C - Peptide	Electro Chemiluminescence
26	CLINICAL BIOCHEMISTRY	Serum	C A 125	Chemiluminescence
27	CLINICAL BIOCHEMISTRY	Serum	C A 15.3	Chemiluminescence
28	CLINICAL BIOCHEMISTRY	Serum	C A 19.9	Chemiluminescence
29	CLINICAL BIOCHEMISTRY	Serum	Calcium	NM-BAPTA
30	CLINICAL BIOCHEMISTRY	Serum	Calcium Ionized	Direct potentiometry ion selective electrode
31	CLINICAL BIOCHEMISTRY	Serum	Carcino Embryonic Antigen	Electro Chemiluminescence
32	CLINICAL BIOCHEMISTRY	Serum	Chloride	Direct Potentiometry Ion Selective Electrode
33	CLINICAL BIOCHEMISTRY	Serum	Cholesterol	CHOD PAP
34	CLINICAL BIOCHEMISTRY	Serum	Cholestrol Non High Density Lipoprotein	Calculated



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

3 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
35	CLINICAL BIOCHEMISTRY	Serum	Cortisol	Electro Chemiluminescence
36	CLINICAL BIOCHEMISTRY	Serum	CPK	Kinetic
37	CLINICAL BIOCHEMISTRY	Serum	Creatine Kinase - MB	Chemiluminescence
38	CLINICAL BIOCHEMISTRY	Serum	Creatinine	Jaffe
39	CLINICAL BIOCHEMISTRY	Serum	DHEA-S	Chemiluminescence
40	CLINICAL BIOCHEMISTRY	Serum	Double Marker Test	Calculated
41	CLINICAL BIOCHEMISTRY	Serum	Estradiol	Chemiluminescence
42	CLINICAL BIOCHEMISTRY	Serum	Ferritin	Electro Chemiluminescence
43	CLINICAL BIOCHEMISTRY	Serum	Folate	Chemiluminescence
44	CLINICAL BIOCHEMISTRY	Serum	Follicle Stimulating Hormone (FSH)	CLIA
45	CLINICAL BIOCHEMISTRY	Serum	Free PSA	Chemiluminescence
46	CLINICAL BIOCHEMISTRY	Serum	Free β Human chorionic gonadotropin	Electro Chemiluminescence
47	CLINICAL BIOCHEMISTRY	Serum	Gamma	Gel Electrophoresis
48	CLINICAL BIOCHEMISTRY	Serum	Gamma Glutamyl Transferase	International Federation of Clinical Chemistry
49	CLINICAL BIOCHEMISTRY	Serum	Growth Hormone	Chemiluminescence
50	CLINICAL BIOCHEMISTRY	Serum	High Density Lipoprotein Cholesterol	Homogeneous Enzymatic Colorimetry
51	CLINICAL BIOCHEMISTRY	Serum	HOMA- IR	Calculated
52	CLINICAL BIOCHEMISTRY	Serum	Homocystein	CLIA
53	CLINICAL BIOCHEMISTRY	Serum	hsCRP	Nephelometry



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

4 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
54	CLINICAL BIOCHEMISTRY	Serum	Immunoglobulin A	Nephelometry
55	CLINICAL BIOCHEMISTRY	Serum	Immunoglobulin E	CLIA
56	CLINICAL BIOCHEMISTRY	Serum	Immunoglobulin G	Immunoturbidimetry
57	CLINICAL BIOCHEMISTRY	Serum	Immunoglobulin M	Immunoturbidimetry
58	CLINICAL BIOCHEMISTRY	Serum	Inhibin A	Chemiluminescence
59	CLINICAL BIOCHEMISTRY	Serum	Insulin	CLIA
60	CLINICAL BIOCHEMISTRY	Serum	Iron	Ferrozine
61	CLINICAL BIOCHEMISTRY	Serum	LDH	IFCC
62	CLINICAL BIOCHEMISTRY	Serum	LDL/HDL Cholesterol Ratio	Calculated
63	CLINICAL BIOCHEMISTRY	Serum	Low Density Lipoprotein Cholesterol	Calculated
64	CLINICAL BIOCHEMISTRY	Serum	Low Density Lipoprotein Cholesterol	Homogeneous Enzymatic Colorimetry
65	CLINICAL BIOCHEMISTRY	Serum	Luteinizing Hormone (LH)	CLIA
66	CLINICAL BIOCHEMISTRY	Serum	NT-Pro BNP	ECLA
67	CLINICAL BIOCHEMISTRY	Serum	PAPP A	Electrochemiluminescence
68	CLINICAL BIOCHEMISTRY	Serum	Para Thyroid Hormone	CLIA
69	CLINICAL BIOCHEMISTRY	Serum	Phenytoin	CLIA
70	CLINICAL BIOCHEMISTRY	Serum	Phosphorus	Molybdate Ultra Violet
71	CLINICAL BIOCHEMISTRY	Serum	Potassium	Direct Potentiometry Ion Selective Electrode
72	CLINICAL BIOCHEMISTRY	Serum	Procalcitonin	ECLIA
73	CLINICAL BIOCHEMISTRY	Serum	Progesterone	CLIA
74	CLINICAL BIOCHEMISTRY	Serum	Prolactin	CLIA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

5 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
75	CLINICAL BIOCHEMISTRY	Serum	Prostate Specific Antigen Total	Chemiluminescence
76	CLINICAL BIOCHEMISTRY	Serum	Quadruple Marker Test	Calculated
77	CLINICAL BIOCHEMISTRY	Serum	Sodium	Direct Potentiometry Ion Selective Electrode
78	CLINICAL BIOCHEMISTRY	Serum	β Human chorionic gonadotropin	Electrochemiluminescence
79	CLINICAL BIOCHEMISTRY	Serum	Testosterone Total	Chemiluminescence
80	CLINICAL BIOCHEMISTRY	Serum	Testosterone, Free	ELISA
81	CLINICAL BIOCHEMISTRY	Serum	Thyroxine Free (FT4)	CLIA
82	CLINICAL BIOCHEMISTRY	Serum	Thyroxine Total (T4)	CLIA
83	CLINICAL BIOCHEMISTRY	Serum	TIBC	Calculated
84	CLINICAL BIOCHEMISTRY	Serum	Total Cholesterol/HDL Cholesterol Ratio	Calculated
85	CLINICAL BIOCHEMISTRY	Serum	Total Protein	Biuret
86	CLINICAL BIOCHEMISTRY	Serum	Transferrin Saturation	Calculated
87	CLINICAL BIOCHEMISTRY	Serum	Tri iodothyronine Free (FT3)	CLIA
88	CLINICAL BIOCHEMISTRY	Serum	Tri iodothyronine total (T3)	CLIA
89	CLINICAL BIOCHEMISTRY	Serum	Triglyceride	Enzymatic
90	CLINICAL BIOCHEMISTRY	Serum	Triple Marker Test	Calculated
91	CLINICAL BIOCHEMISTRY	Serum	TSH	CLIA
92	CLINICAL BIOCHEMISTRY	Serum	Unconjugated Estriol	CLIA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

6 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
93	CLINICAL BIOCHEMISTRY	Serum	Unsaturated Iron Binding Capacity (UIBC)	Ferrozine
94	CLINICAL BIOCHEMISTRY	Serum	Urea	Urease
95	CLINICAL BIOCHEMISTRY	Serum	Uric acid	Uricase
96	CLINICAL BIOCHEMISTRY	Serum	Valproic Acid	CLIA
97	CLINICAL BIOCHEMISTRY	Serum	Very Low Density Lipoprotein	Calculated
98	CLINICAL BIOCHEMISTRY	Serum	Vitamin B12	CLIA
99	CLINICAL BIOCHEMISTRY	Serum	Vitamin D	CLIA
100	CLINICAL BIOCHEMISTRY	Serum, Peritoneal Fluid	Amylase	Enzymatic
101	CLINICAL BIOCHEMISTRY	Serum, Peritoneal fluid	Lipase	Enzymatic colorimetric
102	CLINICAL BIOCHEMISTRY	Urine	Creatinine	Jaffe Kinetic
103	CLINICAL BIOCHEMISTRY	Urine	Microalbumin	Immunoturbidimetry
104	CLINICAL BIOCHEMISTRY	Urine, CSF	Protein	Turbidimetric
105	CLINICAL PATHOLOGY	Pericardial Fluid / CSF / Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Colour	Visual
106	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid / Urine / Stool	Others	Light Microscopy
107	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Appearance	Visual
108	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Blood	Manual



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

7 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
109	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Coagulam	Visual
110	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Lymphocytes	Light Microscopy
111	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Neutrophils	Light Microscopy
112	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	pH	Double Indicator
113	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	TLC	Manual
114	CLINICAL PATHOLOGY	Pericardial Fluid / CSF/ Pleural Fluid / Peritoneal Fluid / Synovial Fluid.	Volume	Visual
115	CLINICAL PATHOLOGY	Semen	Colour	Visual
116	CLINICAL PATHOLOGY	Semen	Epithelial Cells	Light Microscopy
117	CLINICAL PATHOLOGY	Semen	Fructose	Seliwanoff
118	CLINICAL PATHOLOGY	Semen	Liquifaction Time	Manual
119	CLINICAL PATHOLOGY	Semen	Morphology	Eosin, Nigrosin Stain and Light Microscopy
120	CLINICAL PATHOLOGY	Semen	Motility	Light Microscopy
121	CLINICAL PATHOLOGY	Semen	Pus cells	Light Microscopy
122	CLINICAL PATHOLOGY	Semen	RBC	Light Microscopy



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

8 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
123	CLINICAL PATHOLOGY	Semen	Reaction	Double Indicator
124	CLINICAL PATHOLOGY	Semen	Total Sperm Count	Light Microscopy
125	CLINICAL PATHOLOGY	Semen	Viability	Light Microscopy
126	CLINICAL PATHOLOGY	Semen	Viscosity	Visual
127	CLINICAL PATHOLOGY	Semen	Volume	Visual
128	CLINICAL PATHOLOGY	Stool	Blood	Visual
129	CLINICAL PATHOLOGY	Stool	Colour	Visual
130	CLINICAL PATHOLOGY	Stool	Consistency	Visual
131	CLINICAL PATHOLOGY	Stool	Cysts	Light Microscopy
132	CLINICAL PATHOLOGY	Stool	Mucus	Visual
133	CLINICAL PATHOLOGY	Stool	Occult Blood	Immunochromatography
134	CLINICAL PATHOLOGY	Stool	Ova	Light Microscopy
135	CLINICAL PATHOLOGY	Stool	Parasites	Visual
136	CLINICAL PATHOLOGY	Stool	Pus	Visual
137	CLINICAL PATHOLOGY	Stool	Pus Cells	Light Microscopy
138	CLINICAL PATHOLOGY	Stool	Red Blood Cells	Light Microscopy
139	CLINICAL PATHOLOGY	Urine	Pregnancy Test	Immunochemical sandwich assay
140	CLINICAL PATHOLOGY	Urine	Amphetamines	Immunochromatography
141	CLINICAL PATHOLOGY	Urine	Ascorbic acid	Dichlorophenolindophenol
142	CLINICAL PATHOLOGY	Urine	Bacteria	Cuvette Based Microscopy
143	CLINICAL PATHOLOGY	Urine	Bacteria	Light Microscopy



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

9 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
144	CLINICAL PATHOLOGY	Urine	Barbiturates	Immunochemistry
145	CLINICAL PATHOLOGY	Urine	Bence Jones Protein	Precipitation of protein by heat coagulation
146	CLINICAL PATHOLOGY	Urine	Benzodiazepines	Immunochemistry
147	CLINICAL PATHOLOGY	Urine	Bile Pigment	Fouchet's
148	CLINICAL PATHOLOGY	Urine	Bile Salt	Hays Sulphur powder
149	CLINICAL PATHOLOGY	Urine	Bilirubin	Azo-coupling reaction
150	CLINICAL PATHOLOGY	Urine	Blood	Peroxidase
151	CLINICAL PATHOLOGY	Urine	Cast	Cuvette Based Microscopy
152	CLINICAL PATHOLOGY	Urine	Cast	Microscopy
153	CLINICAL PATHOLOGY	Urine	Cocaine	Immunochemistry
154	CLINICAL PATHOLOGY	Urine	Colour	Visual
155	CLINICAL PATHOLOGY	Urine	Cotinine	Immunochemistry
156	CLINICAL PATHOLOGY	Urine	Crystals	Cuvette Based Microscopy
157	CLINICAL PATHOLOGY	Urine	Crystals	Microscopy
158	CLINICAL PATHOLOGY	Urine	Epithelial Cells	Cuvette Based Microscopy
159	CLINICAL PATHOLOGY	Urine	Epithelial cells	Microscopy
160	CLINICAL PATHOLOGY	Urine	Ketone	Legal's
161	CLINICAL PATHOLOGY	Urine	Leukocytes	Esterase activity of granulocytes
162	CLINICAL PATHOLOGY	Urine	Marijuana (CannabisTHC)	Immunochemistry
163	CLINICAL PATHOLOGY	Urine	Metamphetamine	Immunochemistry



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

10 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
164	CLINICAL PATHOLOGY	Urine	Methadone	Immunochemistry
165	CLINICAL PATHOLOGY	Urine	Methylenedioxymethamphetamine (XTC)	Immunochemistry
166	CLINICAL PATHOLOGY	Urine	Morphine	Immunochemistry
167	CLINICAL PATHOLOGY	Urine	Nitrite	Griess reaction
168	CLINICAL PATHOLOGY	Urine	Opiates	Immunochemistry
169	CLINICAL PATHOLOGY	Urine	pH	Double indicator
170	CLINICAL PATHOLOGY	Urine	Phencyclidine phosphate (PCP)	Immunochemistry
171	CLINICAL PATHOLOGY	Urine	Pus Cells	Cuvette Based Microscopy
172	CLINICAL PATHOLOGY	Urine	Pus cells	Light Microscopy
173	CLINICAL PATHOLOGY	Urine	RBCs	Cuvette Based Microscopy
174	CLINICAL PATHOLOGY	Urine	RBCs	Microscopy
175	CLINICAL PATHOLOGY	Urine	Specific Gravity	pKa Change
176	CLINICAL PATHOLOGY	Urine	Sugar	Glucose Oxidase Peroxidase
177	CLINICAL PATHOLOGY	Urine	Transparency	Visual
178	CLINICAL PATHOLOGY	Urine	Tricyclic Antidepressants (TCA)	Immunochemistry
179	CLINICAL PATHOLOGY	Urine	Urine Protein	Error-of-Indicator
180	CLINICAL PATHOLOGY	Urine	Urobilinogen	Erlich's
181	CLINICAL PATHOLOGY	Urine	Volume	Visual



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

11 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
182	CLINICAL PATHOLOGY	Urine	WBCs	Cuvette Based Microscopy
183	CLINICAL PATHOLOGY	Urine	WBCs	Microscopy
184	CYTOPATHOLOGY	Cervical and vaginal smears	Cervico vaginal smear Conventional	PAP staining, Light Microscopy with Interpretation
185	CYTOPATHOLOGY	Cervical and vaginal smears	Cervico vaginal smear, Liquid Based Cytology	Liquid Based Cytology, Light Microscopy with Interpretation
186	CYTOPATHOLOGY	Body Fluids	Cytology	Centrifugation, smear preparation, Giemsa staining and Light Microscopy with Interpretation
187	CYTOPATHOLOGY	Palpable or non palpable lesion involving any organ	Fine Needle Aspiration Cytology	Fine Needle Aspiration Cytology Procedure, smear preparation, Staining with MGG/PAP and Light Microscopy with Interpretation
188	CYTOPATHOLOGY	Slides For Review	Cytology	Light Microscopy with Interpretation
189	CYTOPATHOLOGY	Unstained Slides for Reporting	Cytology	MGG/PAP Staining & Light Microscopy
190	HAEMATOLOGY	EDTA Whole Blood	Absolute Basophil Count	Calculated
191	HAEMATOLOGY	EDTA Whole Blood	Absolute Eosinophil Count	Calculated
192	HAEMATOLOGY	EDTA Whole Blood	Absolute Lymphocyte Count	Calculated



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

12 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
193	HAEMATOLOGY	EDTA Whole Blood	Absolute Monocyte Count	Calculated
194	HAEMATOLOGY	EDTA Whole Blood	Absolute Neutrophil Count	Calculated
195	HAEMATOLOGY	EDTA Whole Blood	Basophils	Double Hydrodynamic Sequential System
196	HAEMATOLOGY	EDTA Whole Blood	Basophils	Leishman's Stain Microscopy
197	HAEMATOLOGY	EDTA Whole Blood	Direct Coombs Test	Gel card agglutination
198	HAEMATOLOGY	EDTA Whole Blood	Eosinophils	Double Hydrodynamic Sequential System
199	HAEMATOLOGY	EDTA Whole Blood	Eosinophils	Leishman's Stain Microscopy
200	HAEMATOLOGY	EDTA Whole Blood	Erythrocytic Sedimentation Rate	Modified Westergren method
201	HAEMATOLOGY	EDTA Whole Blood	G6PD	Enzymatic colorimetry
202	HAEMATOLOGY	EDTA Whole Blood	Haemoglobin	Non Cyanide SLS.
203	HAEMATOLOGY	EDTA Whole Blood	Haemoglobin A1c	High Performance Liquid Chromatography
204	HAEMATOLOGY	EDTA Whole Blood	Haemoglobin A2	High Performance Liquid Chromatography
205	HAEMATOLOGY	EDTA Whole Blood	Haemoglobin adult	High Performance Liquid Chromatography
206	HAEMATOLOGY	EDTA Whole Blood	Haemoglobin Fetal	High Performance Liquid Chromatography
207	HAEMATOLOGY	EDTA Whole Blood	Lymphocytes	Double Hydrodynamic Sequential System



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

13 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
208	HAEMATOLOGY	EDTA Whole Blood	Lymphocytes	Leishman's Stain Microscopy
209	HAEMATOLOGY	EDTA Whole Blood	Mean Corpuscular Haemoglobin	Calculated
210	HAEMATOLOGY	EDTA Whole Blood	Mean Corpuscular Haemoglobin Concentration	Calculated
211	HAEMATOLOGY	EDTA Whole Blood	Mean Corpuscular Volume	Calculated
212	HAEMATOLOGY	EDTA Whole Blood	Monocytes	Double Hydrodynamic Sequential System
213	HAEMATOLOGY	EDTA Whole Blood	Monocytes	Leishman's Stain Microscopy
214	HAEMATOLOGY	EDTA Whole Blood	Neutrophils	Double Hydrodynamic Sequential System
215	HAEMATOLOGY	EDTA Whole Blood	Neutrophils	Leishman's Stain Microscopy
216	HAEMATOLOGY	EDTA Whole Blood	Packed Corpuscular Volume	Cummulative Pulse Height Detection.
217	HAEMATOLOGY	EDTA Whole Blood	Peripheral Blood Smear Examination	Leishman's Stain Microscopy
218	HAEMATOLOGY	EDTA Whole Blood	Peripheral Blood Smear for Malaria Parasite	Leishman's Stain Microscopy
219	HAEMATOLOGY	EDTA Whole Blood	Platelet Count	Electrical Impedence
220	HAEMATOLOGY	EDTA Whole Blood	Platelet count	Leishman's Stain Microscopy
221	HAEMATOLOGY	EDTA Whole Blood	Red Blood Cells Count	Electrical Impedence



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

14 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
222	HAEMATOLOGY	EDTA Whole Blood	Red Cells Distribution Width-CV	Calculated
223	HAEMATOLOGY	EDTA Whole Blood	Reticulocyte Count	Supra Vital Staining (bromocresol blue) & Light Microscopy
224	HAEMATOLOGY	EDTA Whole Blood	Total Leucocyte Count	Electrical Impedence
225	HAEMATOLOGY	EDTA Whole Blood	Total Leucocytes Count	Manual
226	HAEMATOLOGY	Serum	Indirect Coombs Test	Gel card agglutination
227	HAEMATOLOGY	Whole Blood	Blood Group	Slide agglutination (Forward & reverse grouping)
228	HAEMATOLOGY	Whole Blood	Rh type	Slide agglutination
229	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Blood	Aerobic Culture Identification and Drug sensitivity	Automated culture and identification by colorimetry followed by Antibiotic sensitivity by turbidimetry
230	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Blood	Aerobic Culture Identification and Drug sensitivity	Automated culture and identification by conventional method followed by Antibiotic sensitivity by Disc Diffusion
231	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Plasma	IGRA	ELISA
232	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Amoebic serology	ELISA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

15 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
233	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	ANA Blot (17 antigens): dsDNA, Nucleosome, Histone, SmD1, PCNA, PO, SS-A/Ro 60 KD, SS-A/Ro 52 KD, SS-B/La, CENP-B, Scl 70, U1-snRNP, AMA M2, Jo-1, PM-Scl, Mi-2, Ku	Immunoblot
234	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti Beta-2 glycoprotein-1 IgG	ELISA
235	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti Beta-2 glycoprotein-1 IgM	ELISA
236	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti dsDNA antibodies	ELISA
237	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti HBe antibody	ELISA
238	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti HCV antibody	Electro Chemiluminescence
239	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti Nuclear Antibody	ELISA
240	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti Nuclear Antibody	IFA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

16 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
241	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Anti TTG IgA antibody	ELISA
242	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	ASO	Nephelometry
243	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Aspergillus IgG	ELISA
244	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	C-ANCA	ELISA
245	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Cardiolipin IgG antibodies	ELISA
246	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Cardiolipin IgM antibodies	ELISA
247	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Chikungunya IgM antibodies	Lateral flow Chromatographic immunoassy
248	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	CMV IgG	ELISA
249	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	CMV IgM	ELISA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

17 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
250	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Complement 3	Nephelometry
251	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Complement 4	Nephelometry
252	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	COVID 19 TOTAL ANTIBODY	ECLA
253	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	CRP	Immunoturbidimetry
254	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Dengue NS 1 antigen	Immunochemistry
255	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Dengue Serology IgG	Immunochemistry
256	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Dengue Serology IgM	Immunochemistry
257	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HAV - IgG	ELISA
258	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HAV - IgM	ELISA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

18 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
259	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HBcAb-IgM	ELISA
260	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HBcAb-Total	ELISA
261	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HBeAg	ELISA
262	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HBsAb	ELISA
263	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HBsAg	Electro chemiluminescence
264	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HEV - IgM	ELISA
265	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HEV IgG	ELISA
266	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HIV	Immuno Chromatography
267	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HIV	Immunofiltration



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

19 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
268	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HIV Duo	Electro Chemiluminescence
269	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-1 & 2 IgG	ELISA
270	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-1 & 2 IgM	ELISA
271	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-1 IgG	ELISA
272	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-1 IgM	ELISA
273	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-2 IgG	ELISA
274	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	HSV-2 IgM	ELISA
275	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Hydatid Serology	ELISA
276	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Leptospira antibodies IgM	ELISA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

20 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
277	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	P-ANCA	ELISA
278	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Phospholipid IgG	ELISA
279	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Phospholipid IgM	ELISA
280	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	RA Factor	Immunoturbidimetry
281	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Rapid test for syphilis	Immuno chromatography
282	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Rubella IgG	ELISA
283	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Rubella IgM	ELISA
284	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Scrub Typhus IgM	Immunochromatography
285	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Toxoplasma IgG	ELISA



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

21 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
286	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Toxoplasma IgM	ELISA
287	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	TPHA	Tube agglutination
288	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Typhidot- IgG	Lateral flow Chromatographic immunoassy
289	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Typhidot- IgM	Lateral flow Chromatographic immunoassy
290	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum	Widal	Direct Agglutination
291	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Serum/ BAL fluid	Galactomannan Aspergillus Antigen	ELISA
292	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Sputum, BAL, E.T/T.T Secretions, Bronchial Wash, Pus, Urine, Stool, CSF, Ascitic Fluid, Pericardial Fluid, Pleural Fluid, Synovial Fluid, Semen, Tissue & Fine Needle aspiration	Gram staining	Manual staining & Microscopy



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

22 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
293	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Sputum, BAL, E.T/T.T Secretions, Bronchial Wash, Pus, Urine, Stool, CSF, Ascitic Fluid, Pericardial Fluid, Pleural Fluid, Synovial Fluid, Semen, Tissue & Fine Needle aspiration	ZN stain	Manual staining & Microscopy
294	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Sputum, BAL, E.T/T.T Secretions, Bronchial Wash, Pus,Urine, Stool, Pus swab, Eye Swab, Ear Swab, Urine, CSF, Ascitic Fluid, Pericardial Fluid, Pleural Fluid, Synovial Fluid, Semen, Tissue, Nasal Material, Sinus Material, Vaginal Secretion.	Aerobic Culture Identification and Drug sensitivity	Conventional culture and identification by colorimetry followed by Sensitivity by turbidimetry
295	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Sputum, BAL, E.T/T.T Secretions, Bronchial Wash, Pus,Urine, Stool, Pus swab, Eye Swab, Ear Swab, Urine, CSF, Ascitic Fluid, Pericardial Fluid, Pleural Fluid, Synovial Fluid, Semen, Tissue, Nasal Material, Sinus Material, Vaginal Secretion.	Aerobic Culture Identification and Drug sensitivity	Conventional culture and identification followed by Sensitivity by Disc Diffusion



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

23 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
296	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Sputum, BAL, E.T/T.T Secretions, Bronchial Wash, Pus,Urine, Stool, Pus swab, Throat Swab, Eye Swab, Ear Swab, Urine, CSF, Ascitic Fluid, Pericardial Fluid, Pleural Fluid, Synovial Fluid, Semen, Tissue, Nail, Hair, Skin,Nasal Material, Sinus Material, Vaginal Secretion, Urethral Smear	Fungal smear	KOH prepration & Microscopy
297	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Throat Swab	Aerobic Culture Identification and Drug sensitivity	Conventional culture and identification and Sensitivity followed by Disc Diffusion
298	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Throat swab	Aerobic Culture Identification and Drug sensitivity	conventional culture and identification by colorimetry followed by Antibiotic sensitivity by turbidimetry
299	MICROBIOLOGY & INFECTIOUS DISEASE SEROLOGY	Whole Blood	Malaria Antigen detection 1. Plasmodium Vivax 2. Plasmodium Falciparum	Immuno-chromatography (HRP-II and pLDH)
300	MOLECULAR TESTING	Ascitic fluid, Pleural fluid, Pus, Sputum, Tissue, BAL fluid, CSF, Peritoneal fluid, Lymph node aspirate	AFB Expert panel	Nested real-time PCR



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

24 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
301	MOLECULAR TESTING	Cervical brushing	HPV High Risk Genotyping, Type 16, Type 18 and Type Other Than 16 and 18	Real Time PCR
302	MOLECULAR TESTING	EDTA Plasma	Hepatitis B Viral Load	Real Time PCR
303	MOLECULAR TESTING	EDTA Plasma	Hepatitis B Virus Qualitative	Real Time PCR
304	MOLECULAR TESTING	EDTA Plasma	Hepatitis C RNA Quantitative	Real Time RT PCR (Open System)
305	MOLECULAR TESTING	EDTA Plasma	Hepatitis C Virus Genotyping, Type 1, Type 1b, Type 2, Type 3, Type 4, Type 5 and Type 6	Real Time RT PCR (Open System)
306	MOLECULAR TESTING	EDTA Plasma	Hepatitis C Virus RNA Qualitative	Real Time RT PCR (Open System)
307	MOLECULAR TESTING	EDTA Plasma	HIV-I RNA Qualitative	Real Time RT PCR (Open System)
308	MOLECULAR TESTING	EDTA Plasma	HIV-I RNA Quantitative	Real Time RT PCR (Open System)
309	MOLECULAR TESTING	EDTA Whole Blood	HLA-B27	Real Time PCR
310	MOLECULAR TESTING	EDTA Whole Blood, CSF, Menstrual blood, Tissue in Saline/Formaline, Paraffin Block, Sputum, Body Fluids, FNA Material, Urine, Pus, BAL fluid, Gastric lavage	Mycobacterium Tuberculosis	Real Time PCR



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

25 of 33


Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

S.No	Discipline / Group	Materials or Products tested	Component, parameter or characteristic tested / Specific Test Performed / Tests or type of tests performed	Test Method Specification against which tests are performed and / or the techniques / equipment used
311	MOLECULAR TESTING	Nasopharyngeal and oropharyngeal swab	SARS-CoV-2 RNA Qualitative	Real Time RT PCR (Open System)

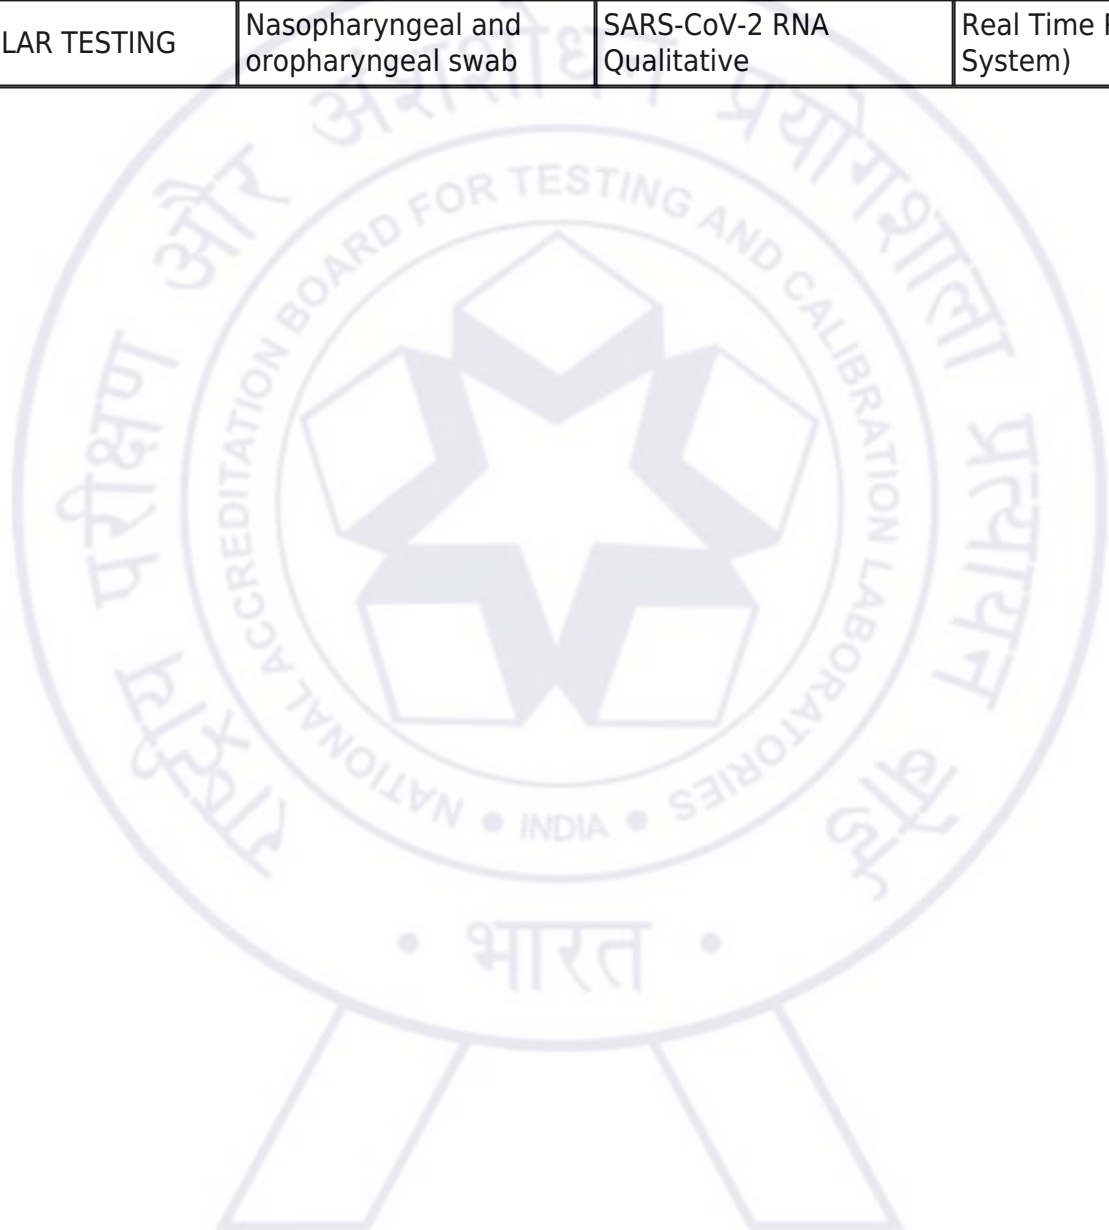



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

26 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002294	International Fertility Centre, Green Park Main	H-6, 1st Floor, Green Park Main, New Delhi, Delhi 110016



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :	PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA		
Accreditation Standard	ISO 15189:2012		
Certificate Number	MC-2270	Page No	27 of 33
Validity	30/06/2021 to 29/06/2023	Last Amended on	12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002298	Dr Gill Path Labs, Amritsar	House Number 98 Sector 4, Ranjit Avenue, Amritsar - 143001, Opposite Chawla



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

28 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002299	Dr Puri Lab, Majitha Road	19, Majitha Road, Medical Enclave, Amritsar - 143001



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :	PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA		
Accreditation Standard	ISO 15189:2012		
Certificate Number	MC-2270	Page No	29 of 33
Validity	30/06/2021 to 29/06/2023	Last Amended on	12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002300	KD Hospital, Amritsar	7, Mental Hospital Road, Amritsar (Pb.) - 143001



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :	PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA		
Accreditation Standard	ISO 15189:2012		
Certificate Number	MC-2270	Page No	30 of 33
Validity	30/06/2021 to 29/06/2023	Last Amended on	12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002301	Malik X-ray and Pathology, Inside Tulip Hospital, Sonipat	Malik X-ray and Pathology, Inside Tulip Hospital, T. P. Scheme no.15, Vivekanand chowk, Delhi road, Sonipat, Haryana 131001



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :	PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA		
Accreditation Standard	ISO 15189:2012		
Certificate Number	MC-2270	Page No	31 of 33
Validity	30/06/2021 to 29/06/2023	Last Amended on	12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002302	Manglam Diagnostics, Hisar	Jindal Hospital Road, Opposite Manglam Blood Bank,, Adjacent Manglam Nuclear Center, Model Town, Hisar Haryana 125005



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :	PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI, DELHI, INDIA		
Accreditation Standard	ISO 15189:2012		
Certificate Number	MC-2270	Page No	32 of 33
Validity	30/06/2021 to 29/06/2023	Last Amended on	12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0002303	Nalwa Pathology and Microbiology Lab, Hisar	SCF 83, Red Square market, Hisar, Haryana 125001



National Accreditation Board for Testing and Calibration Laboratories

SCOPE OF ACCREDITATION

Laboratory Name :

PROGNOSIS LABORATORIES, 515-516, SECTOR-19, DWARKA, NEW DELHI,
DELHI, INDIA

Accreditation Standard

ISO 15189:2012

Certificate Number

MC-2270

Page No

33 of 33

Validity

30/06/2021 to 29/06/2023

Last Amended on

12/07/2021

Recognised Sample Collection Center/Facility

ID of Sample Collection Center / Facility	Name of Sample Collection Center / Facility, Location	Address of Sample Collection Center / Facility
0004454	KKR imaging and diagnostic center, Gurugram	7, Jharsa Rd, Sector 10, Gurugram, Haryana 122007